



INFORMATIONEN ZUR NEUEN SOFTWARE-VERSION 44 DES RAYOCOMP PS 1000 POLAR 4.0

Wenn die neue Vollversion Nr. 44 auf dem Rayocomp PS 1000 polar 4.0 mit dem Modul Rayoscan® installiert wurde, wird automatisch auch der Leistungsumfang des neuen Rayoscan® Humanbereich / Veterinärbereich nutzbar.


Im Falle, dass der Leistungsumfang des Rayoscan® auf die Software-Version 42 zurückgesetzt werden soll, müssen folgende Optionen im Rayocomp PS 1000 polar 4.0 angewählt werden:

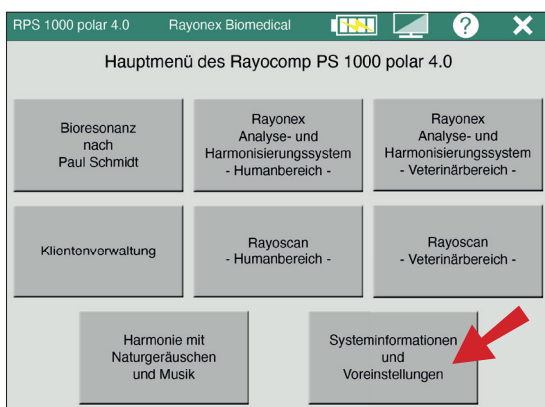


✗ Hauptmenü -
Systeminformationen und Voreinstellungen

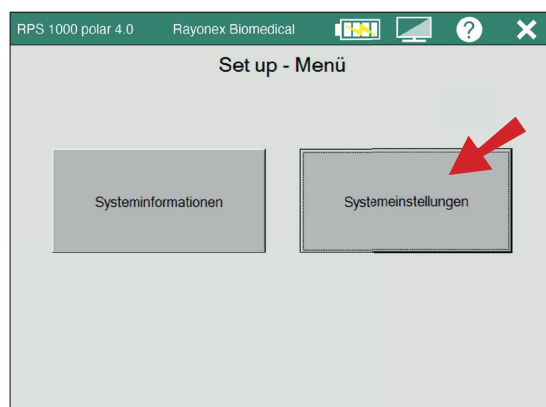

✗ Systemeinstellungen

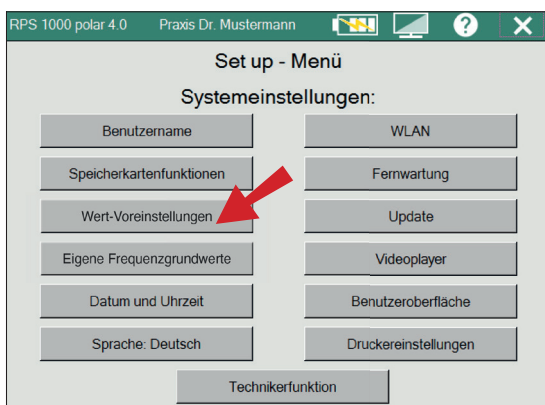

✗ Wert-Voreinstellungen

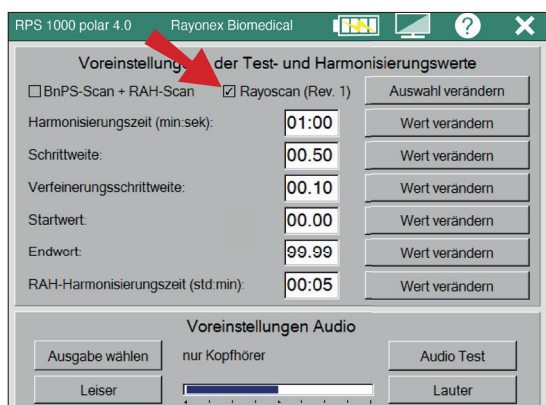

Bitte den Haken wie im Bild setzen, um zum Leistungsumfang der Software-Version 42 zurück zu gelangen.
Dann über das Kreuz das Fenster schließen.



Rayonex Biomedical GmbH

Sauerland-Pyramiden 1 | 57368 Lennestadt


Telefon: 02721 6006-0 | Telefax: 02721 6006-66 | E-Mail: info@rayonex.de

91007DE | Rev000 | Stand: 03. November 2021


INFORMATION ON THE NEW SOFTWARE VERSION 44 OF THE RAYOCOMP PS 1000 POLAR 4.0

If the new full software version no. 44 has been installed on the Rayocomp PS 1000 polar 4.0 where the module Rayoscan®. module is installed, the scope of the new Rayoscan® human / veterinary veterinary area can be used.


In case, that the scope of performance of the Rayoscan is to be reset to software version 42, the following options must be selected in the Rayocomp PS 1000 polar 4.0.

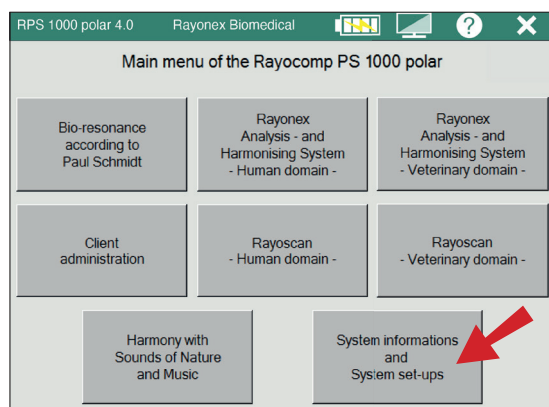


✗ Main menu -
System informations and System set-ups

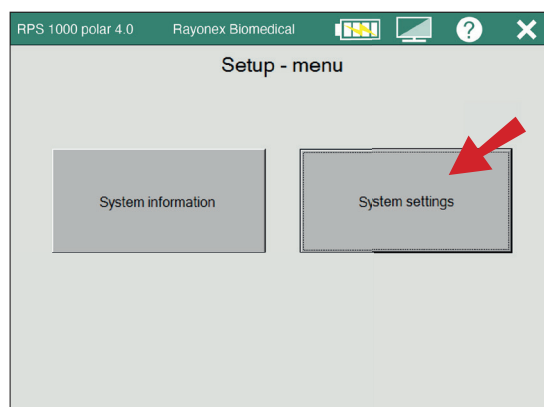

✗ System settings

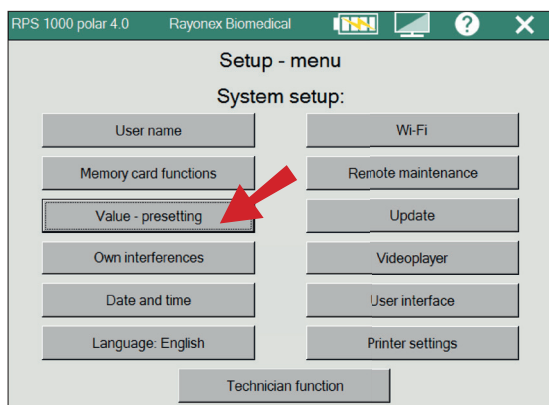

✗ Value - presetting

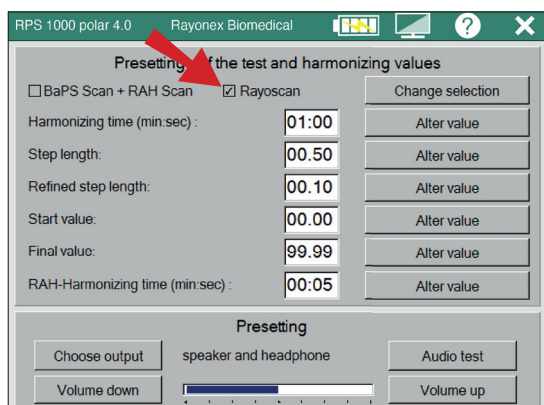

Please tick the box as shown in the image to access the scope of performance of the software version 42 back.
Then close the window by clicking on the X.



Rayonex Biomedical GmbH

Sauerland-Pyramiden 1 | 57368 Lennestadt

Telefon: 02721 6006-0 | Telefax: 02721 6006-66 | E-Mail: info@rayonex.de

91007DE | Rev000 | Stand: 03. November 2021